



SYSTEM INTERCONNECT

(Without facility water & Non Equipment room-400V, Fixed table)

NOTES:

- 1 Customer furnished
- 2 Magnet and superconducting shim power supplies are not included with system, but may remain in place if purchased as an option.
- 3 Dotted line can be available, in the case of Common Ground is installed.
- 4 Typical connection for normally closed emergency off switch.
- 5 Optional: May not be present on all systems.
- 6 Magnet ramping cables pass through rampout on PP1 plate.
- 7 RUNS(600 SERIES) Furnished with GE Magnet.
- 8 RUNS 823 To 833 Furnished Magnet Monitoring.
- 9 Body Hybrid To Body Coil Connections depend on magnet field polarity.
- 10 Customer supplied telephone line for Insite Modem.
- 11 Ethernet cable is customer supplied. RUN E3045 and modem may not be required if connection to Insite is provided through site ethernet connection.
- 12 J1000 is on the Mounting Plate of the Magnet Side Kit
- 13 This cable is for 16 channel system

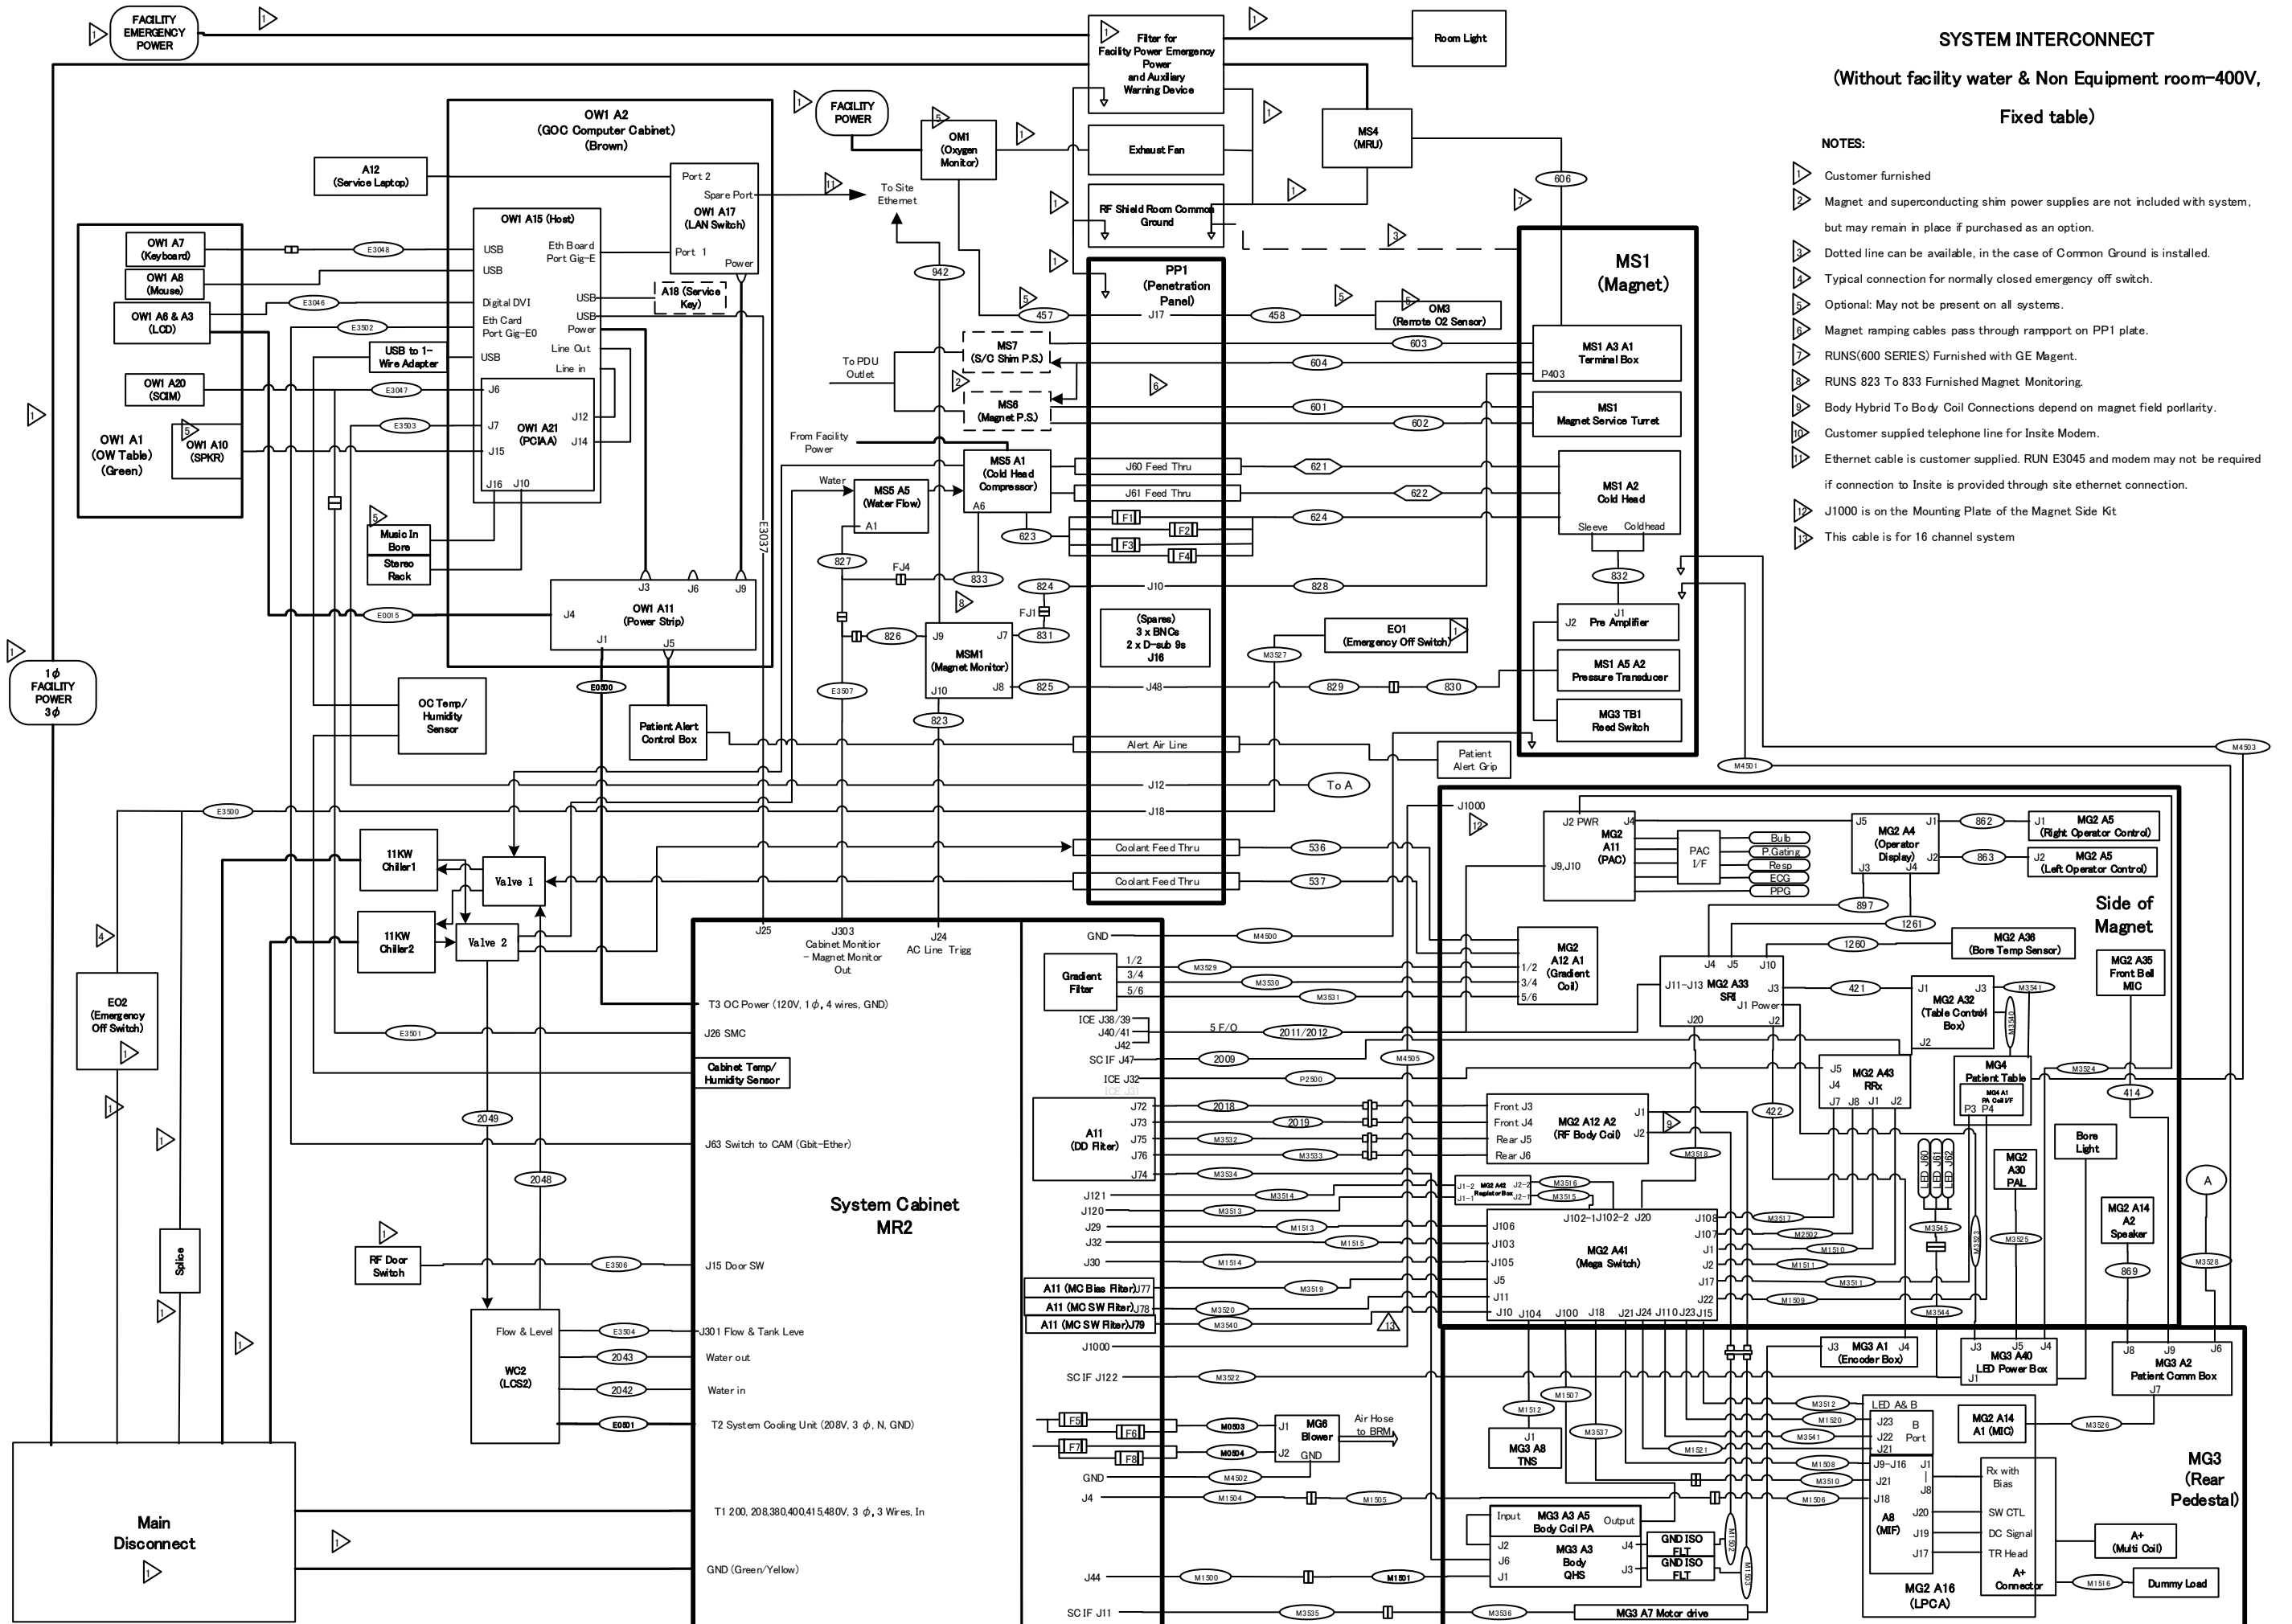

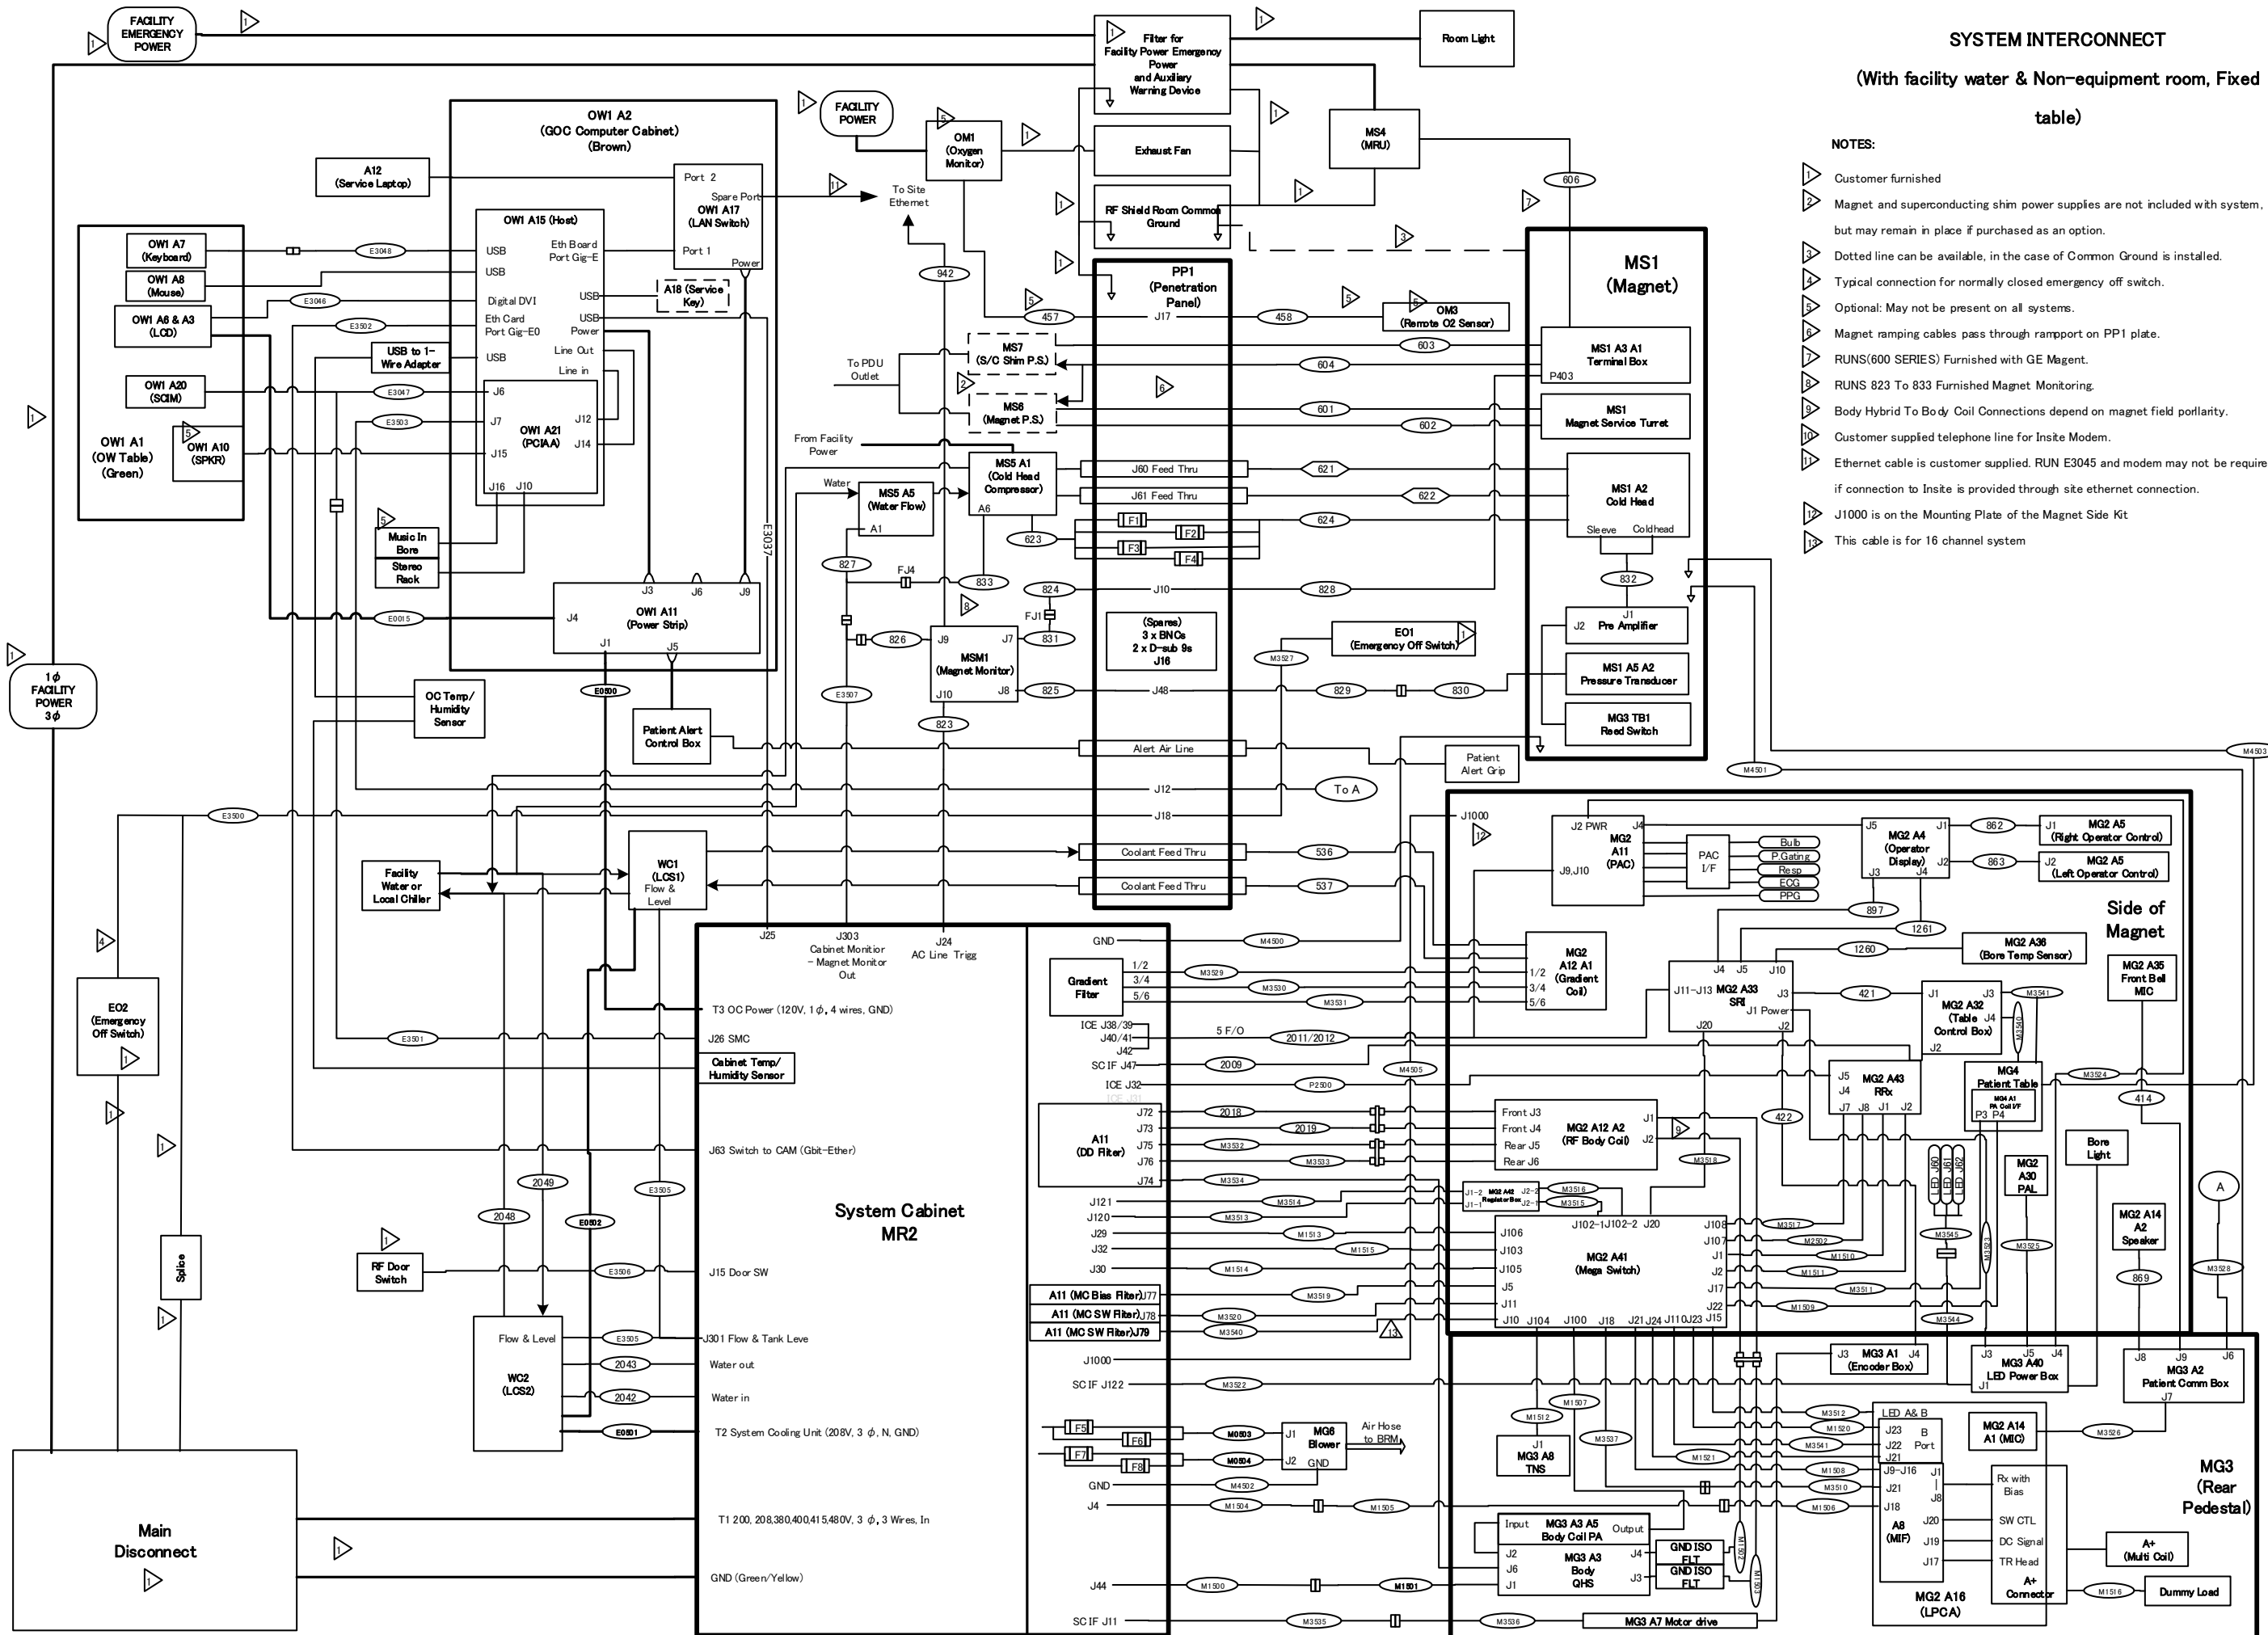


SYSTEM INTERCONNECT

(With facility water & Non-equipment room, Fixed table)

NOTES:

- 1 Customer furnished
- 2 Magnet and superconducting shim power supplies are not included with system, but may remain in place if purchased as an option.
- 3 Dotted line can be available, in the case of Common Ground is installed.
- 4 Typical connection for normally closed emergency off switch.
- 5 Optional: May not be present on all systems.
- 6 Magnet ramping cables pass through rampout on PP1 plate.
- 7 RUNS(600 SERIES) Furnished with GE Magnet.
- 8 RUNS 823 To 833 Furnished Magnet Monitoring.
- 9 Body Hybrid To Body Coil Connections depend on magnet field porlarity.
- 10 Customer supplied telephone line for Insite Modem.
- 11 Ethernet cable is customer supplied. RUN E3045 and modem may not be required if connection to Insite is provided through site ethernet connection.
- 12 J1000 is on the Mounting Plate of the Magnet Side Kit
- 13 This cable is for 16 channel system

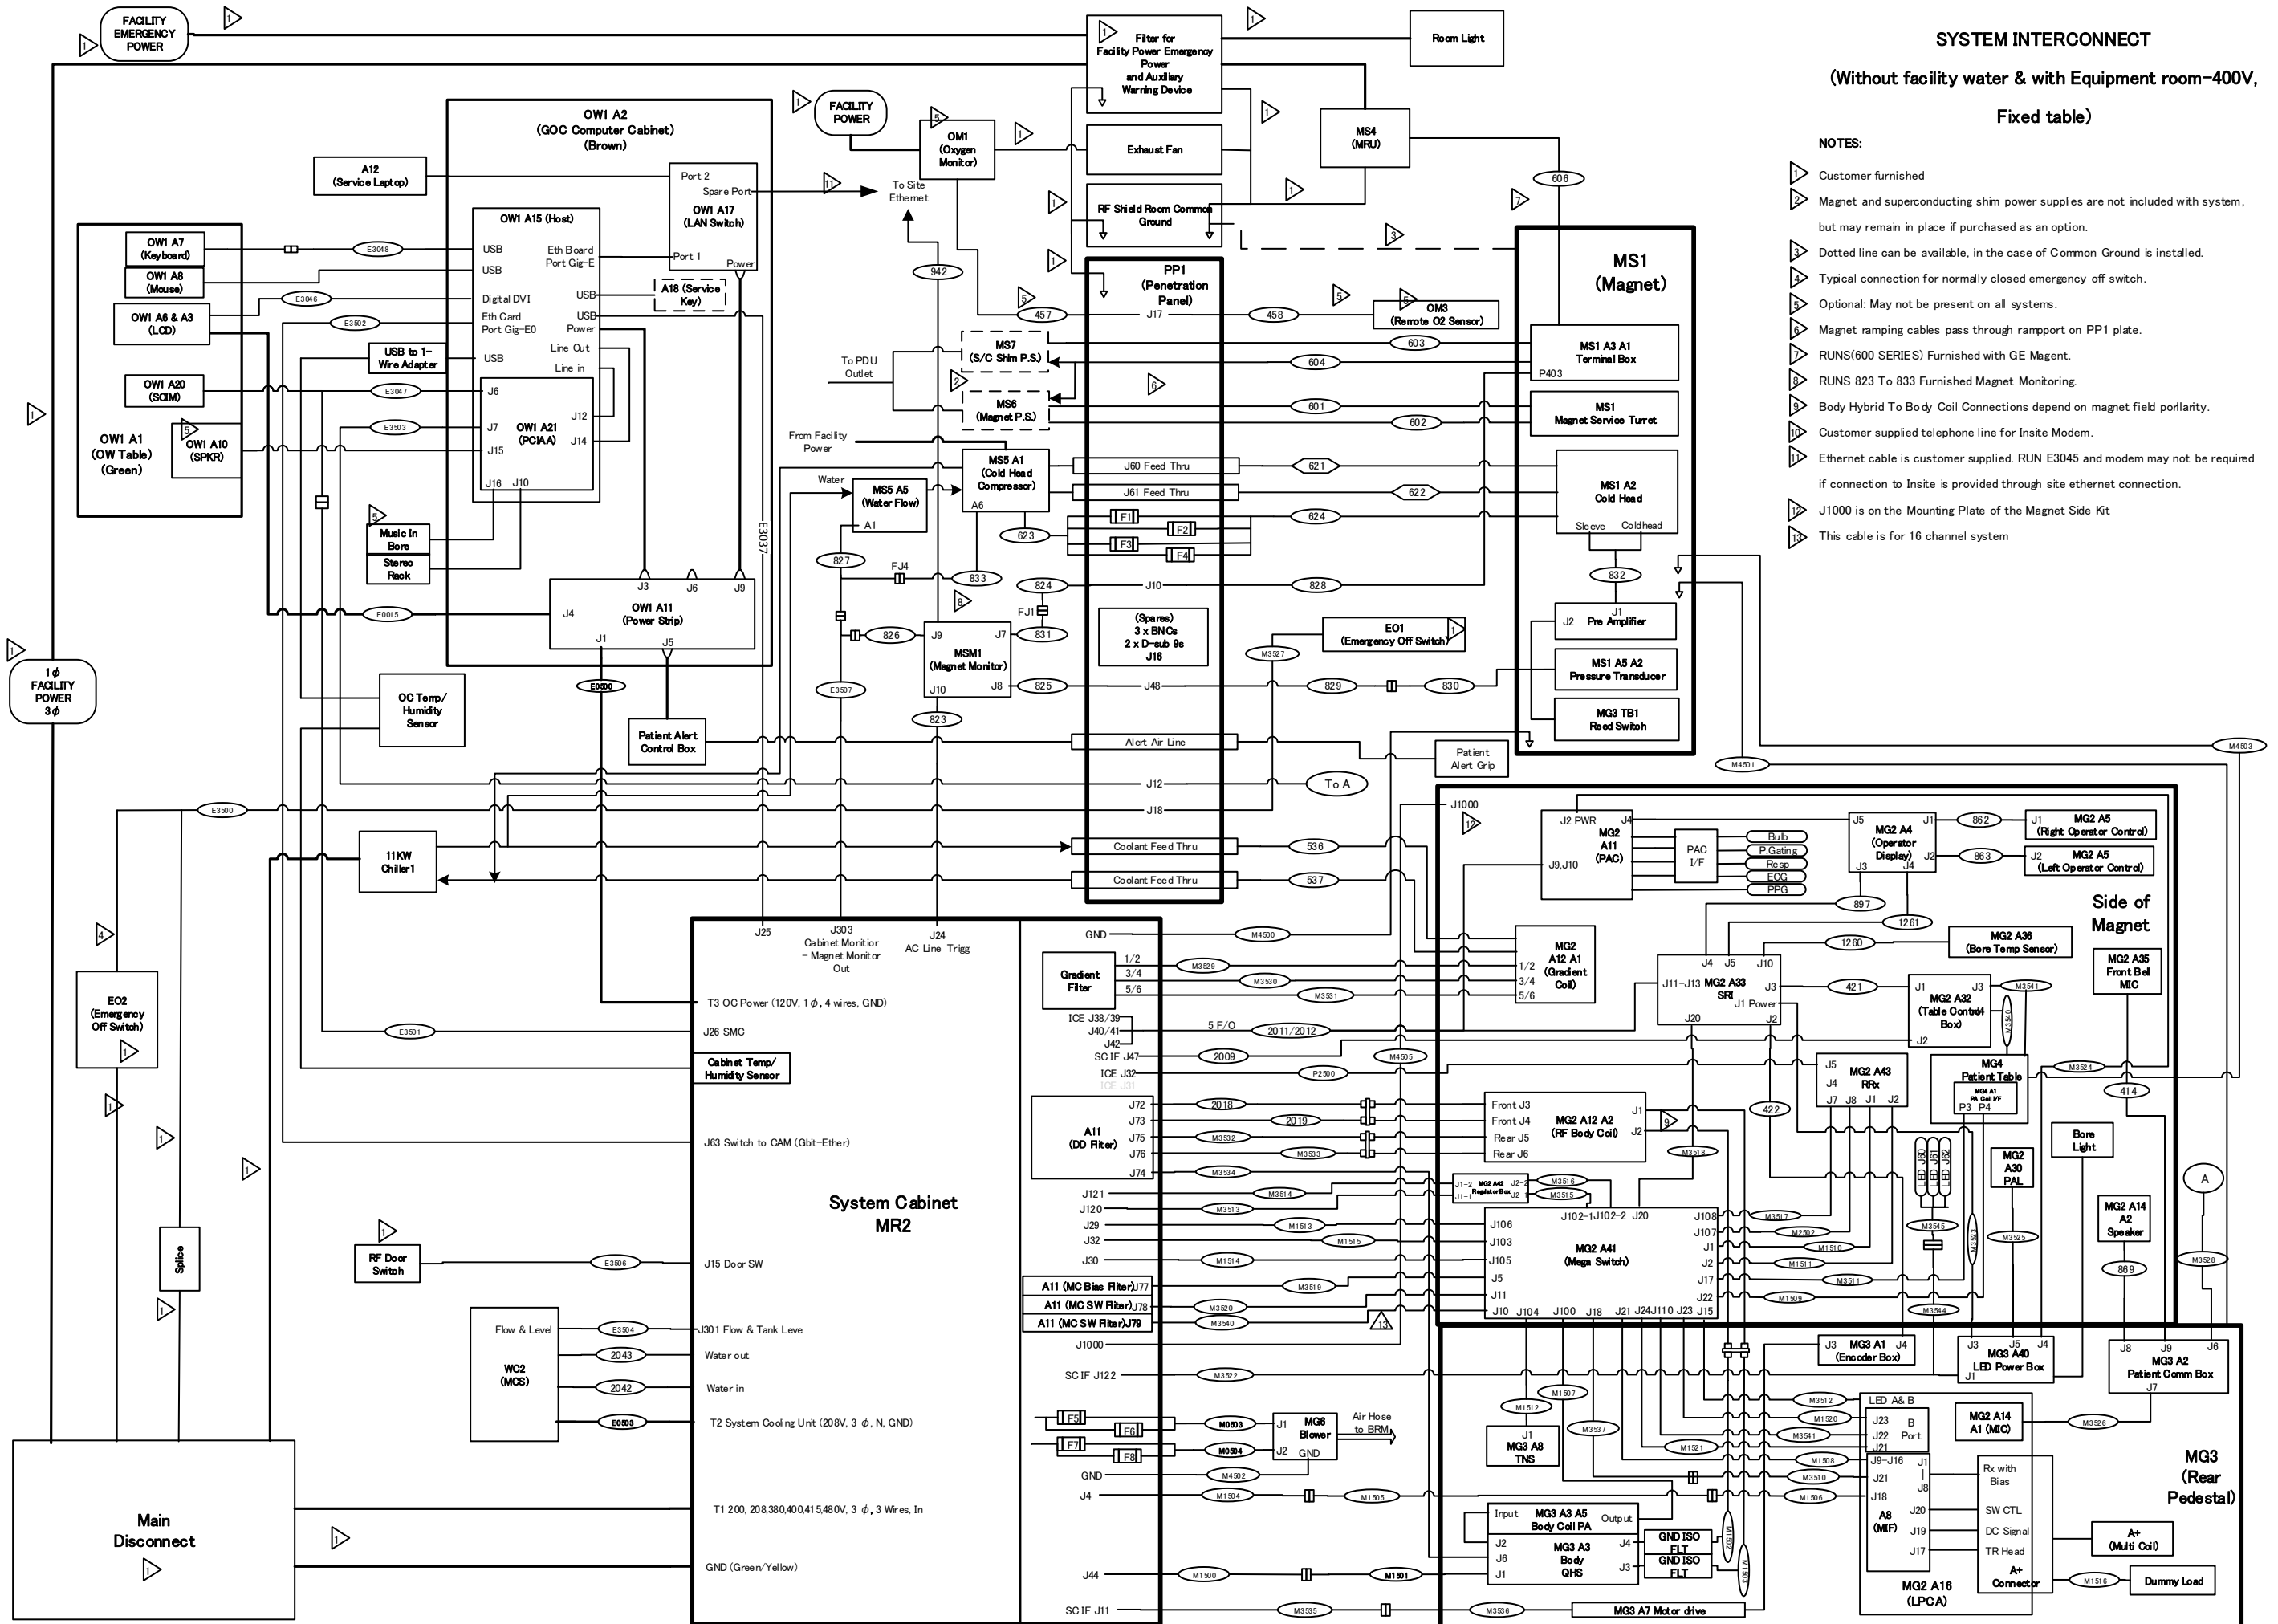

SYSTEM INTERCONNECT

(Without facility water & with Equipment room-400V, Fixed table)

NOTES:


- 1 Customer furnished
- 2 Magnet and superconducting shim power supplies are not included with system, but may remain in place if purchased as an option.
- 3 Dotted line can be available, in the case of Common Ground is installed.
- 4 Typical connection for normally closed emergency off switch.
- 5 Optional: May not be present on all systems.
- 6 Magnet ramping cables pass through rampout on PP1 plate.
- 7 RUNS(600 SERIES) Furnished with GE Magnet.
- 8 RUNS 823 To 833 Furnished Magnet Monitoring.
- 9 Body Hybrid To Body Coil Connections depend on magnet field portlarity.
- 10 Customer supplied telephone line for Insite Modem.
- 11 Ethernet cable is customer supplied. RUN E3045 and modem may not be required if connection to Insite is provided through site ethernet connection.
- 12 J1000 is on the Mounting Plate of the Magnet Side Kit
- 13 This cable is for 16 channel system


SYSTEM INTERCONNECT

(Without facility water & with Equipment room, Fixed table)

NOTES:

- 1 Customer furnished
- 2 Magnet and superconducting shim power supplies are not included with system, but may remain in place if purchased as an option.
- 3 Dotted line can be available, in the case of Common Ground is installed.
- 4 Typical connection for normally closed emergency off switch.
- 5 Optional: May not be present on all systems.
- 6 Magnet ramping cables pass through rampport on PP1 plate.
- 7 RUNS(600 SERIES) Furnished with GE Magent.
- 8 RUNS 823 To 833 Furnished Magnet Monitoring.
- 9 Body Hybrid To Body Coil Connections depend on magnet field porlarity.
- 10 Customer supplied telephone line for Insite Modem.
- 11 Ethernet cable is customer supplied. RUN E3045 and modem may not be required if connection to Insite is provided through site ethernet connection.
- 12 J1000 is on the Mounting Plate of the Magnet Side Kit
- 13 This cable is for 16 channel system

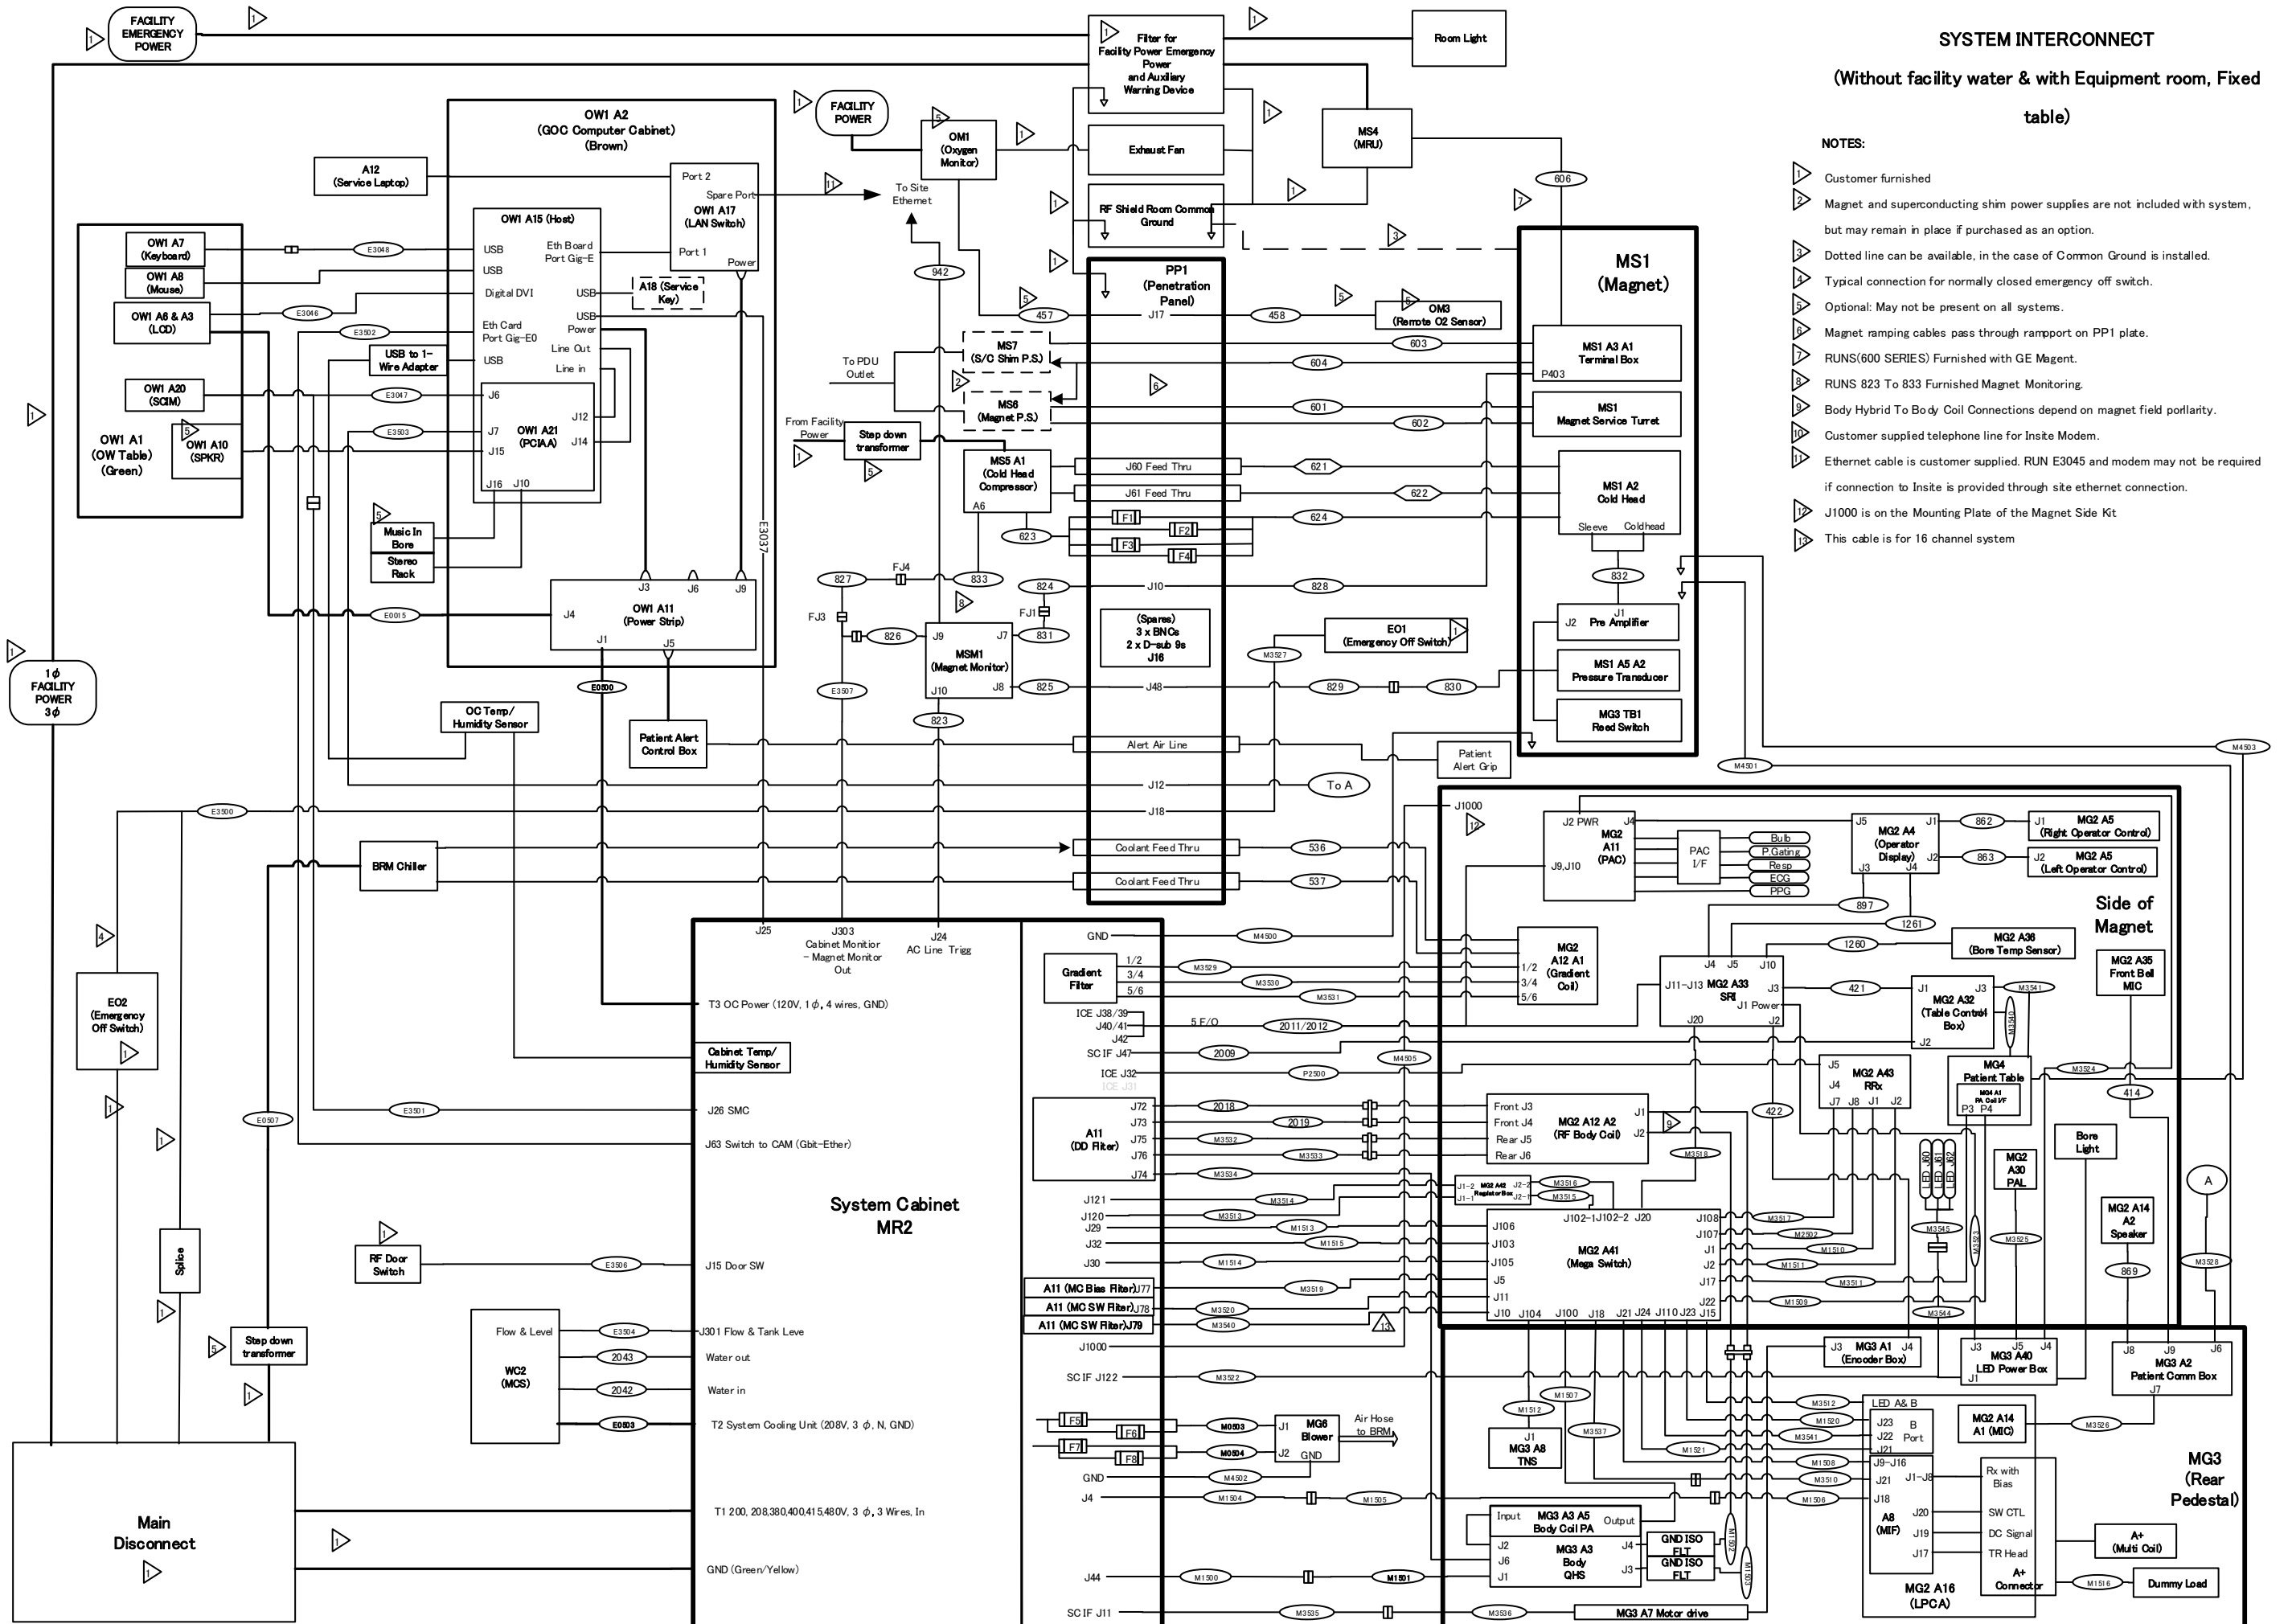

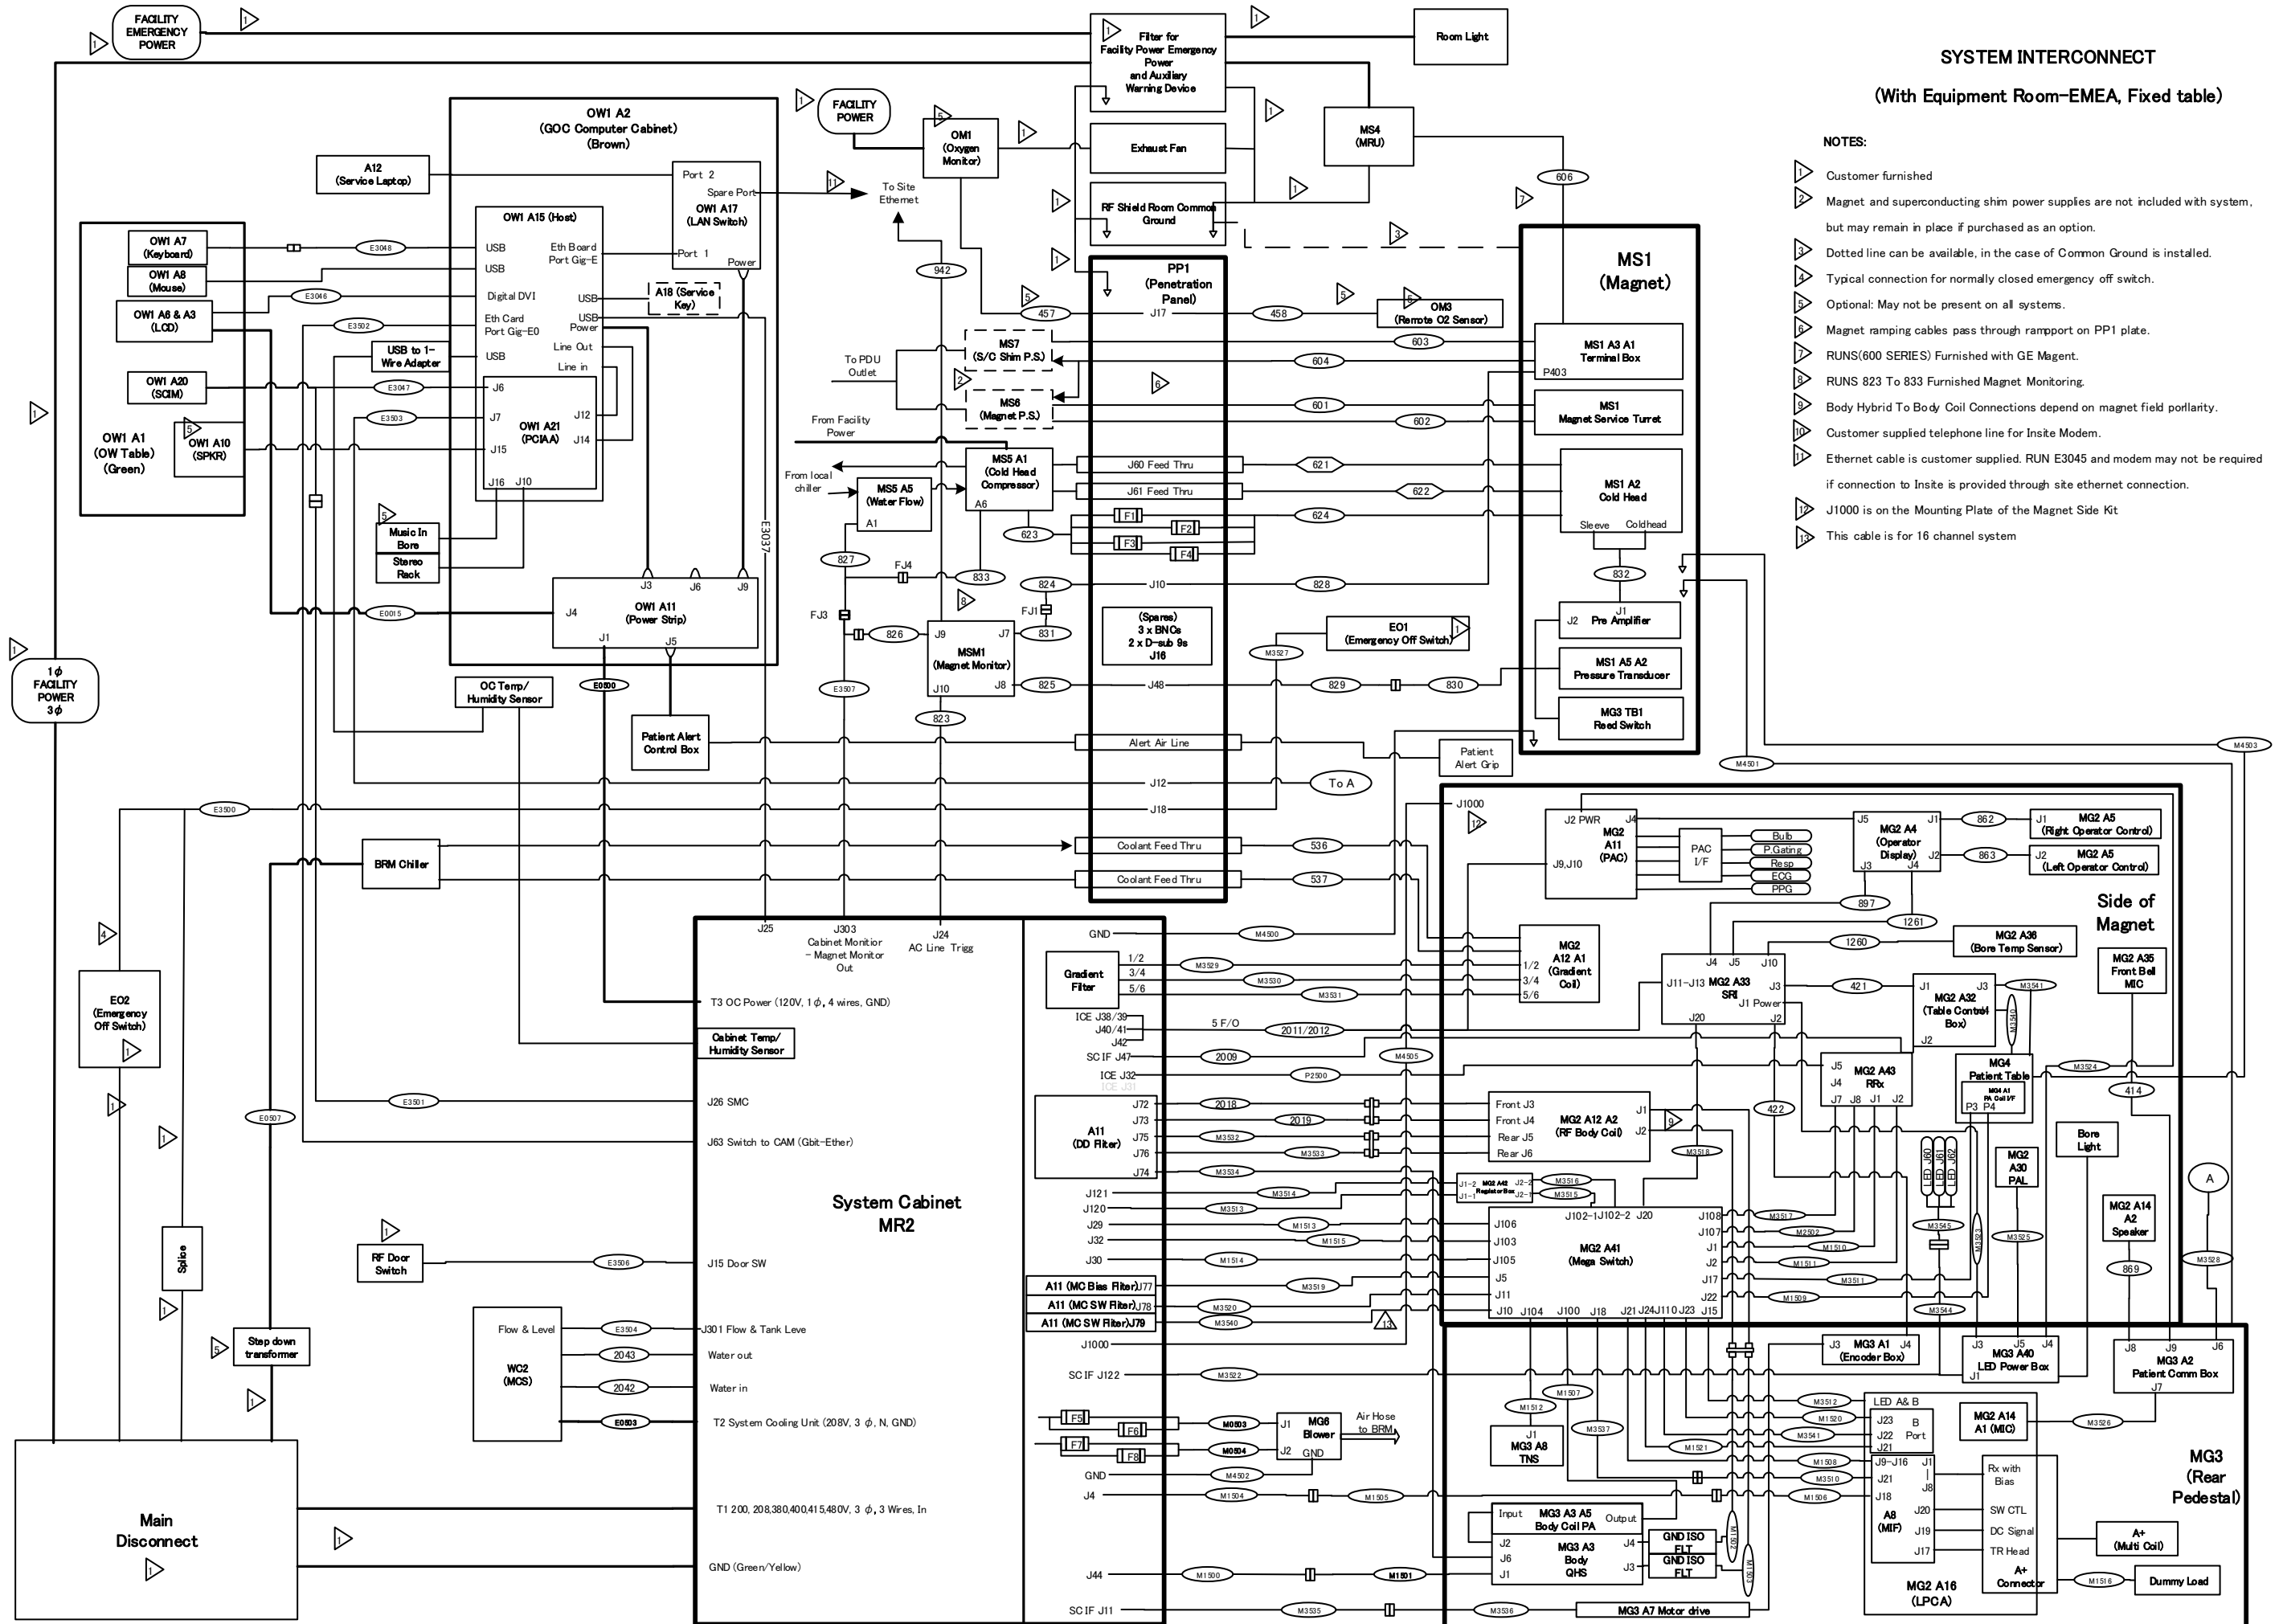

SYSTEM INTERCONNECT
(With Equipment Room-EMEA, Fixed table)

- NOTES:**
- 1 Customer furnished
 - 2 Magnet and superconducting shim power supplies are not included with system, but may remain in place if purchased as an option.
 - 3 Dotted line can be available, in the case of Common Ground is installed.
 - 4 Typical connection for normally closed emergency off switch.
 - 5 Optional: May not be present on all systems.
 - 6 Magnet ramping cables pass through rampout on PP1 plate.
 - 7 RUNS(600 SERIES) Furnished with GE Magnet.
 - 8 RUNS 823 To 833 Furnished Magnet Monitoring.
 - 9 Body Hybrid To Body Coil Connections depend on magnet field polarity.
 - 10 Customer supplied telephone line for Insite Modem.
 - 11 Ethernet cable is customer supplied. RUN E3045 and modem may not be required if connection to Insite is provided through site ethernet connection.
 - 12 J1000 is on the Mounting Plate of the Magnet Side Kit
 - 13 This cable is for 16 channel system