



SYSTEM INTERCONNECT

(Without facility water & with Equipment room,  
Fixed table)

NOTES:

- 1 Customer furnished
- 2 Magnet and superconducting shim power supplies are not included with system, but may remain in place if purchased as an option.
- 3 Dotted line can be available, in the case of Common Ground is installed.
- 4 Typical connection for normally closed emergency off switch.
- 5 Optional: May not be present on all systems.
- 6 Magnet ramping cables pass through rampport on PP1 plate.
- 7 RUNS(600 SERIES) Furnished with GE Magent.
- 8 RUNS 823 To 833 Furnished Magnet Monitoring.
- 9 Body Hybrid To Body Coil Connections depend on magnet field porllarity.
- 10 Customer supplied telephone line for Insite Modem.
- 11 Ethernet cable is customer supplied. RUN E3045 and modem may not be required if connection to Insite is provided through site ethernet connection.
- 12 J1000 is on the Mounting Plate of the Magnet Side Kit
- 13 This cable is for 16 channel system

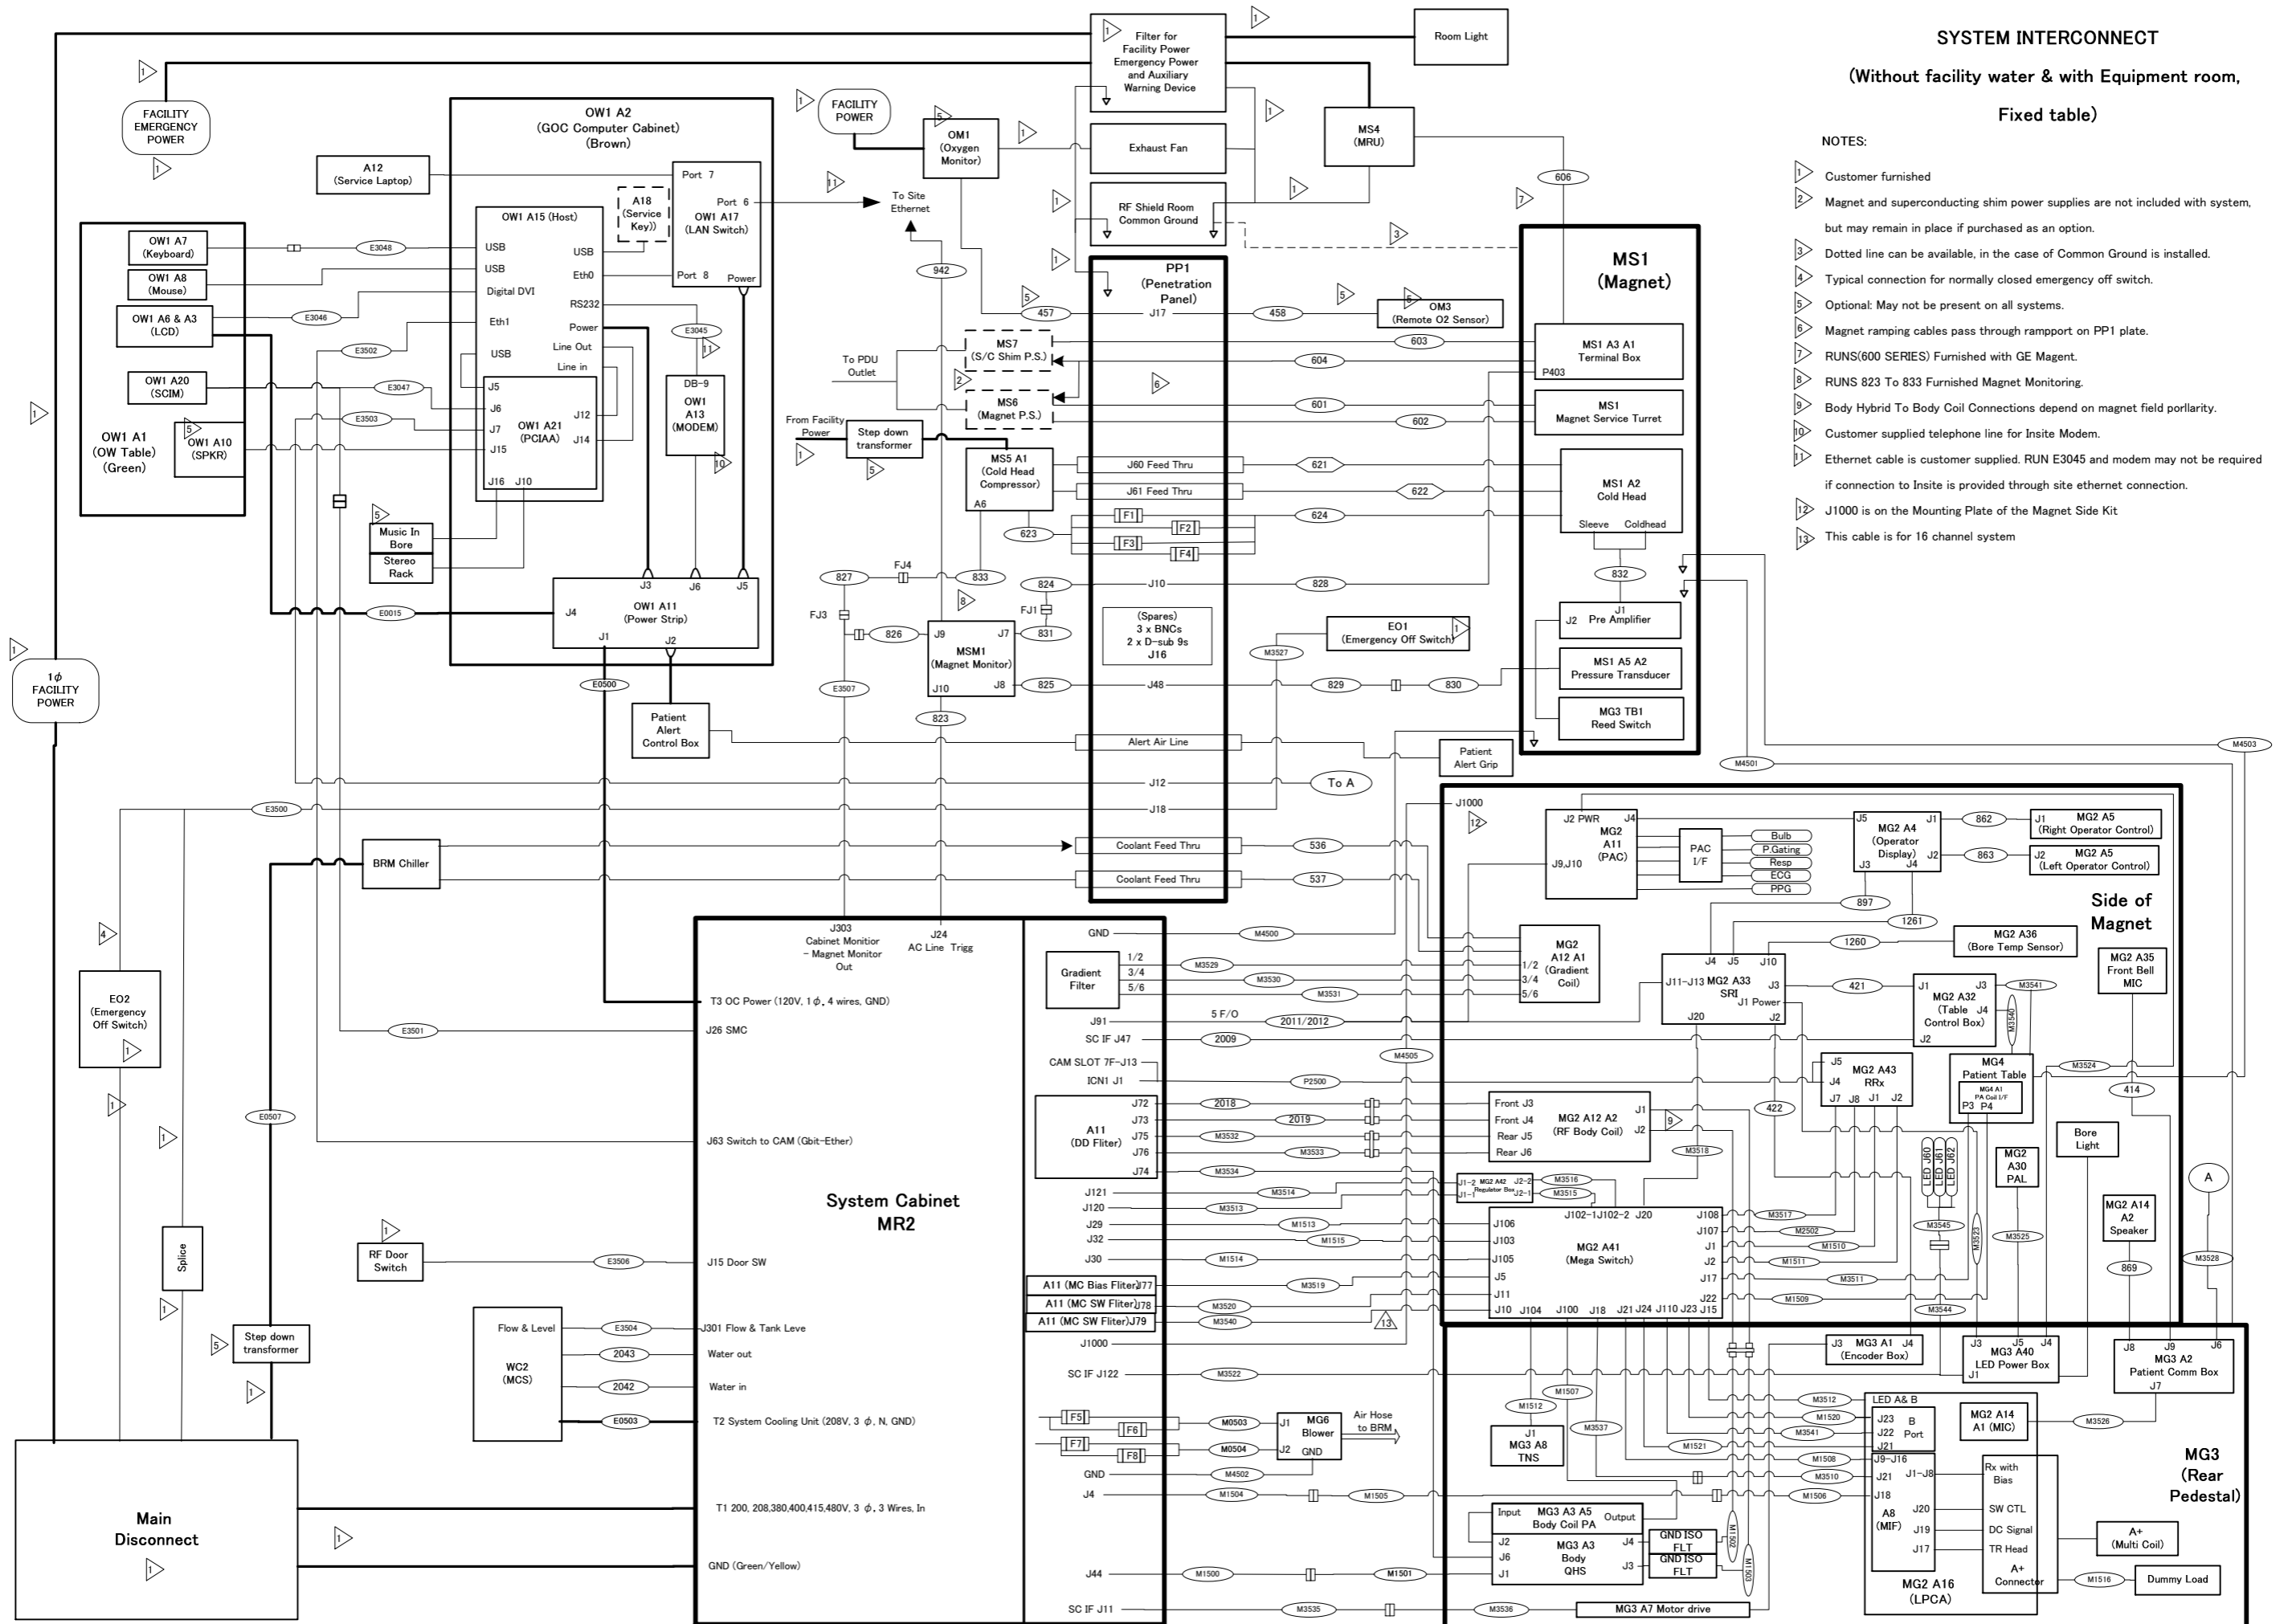

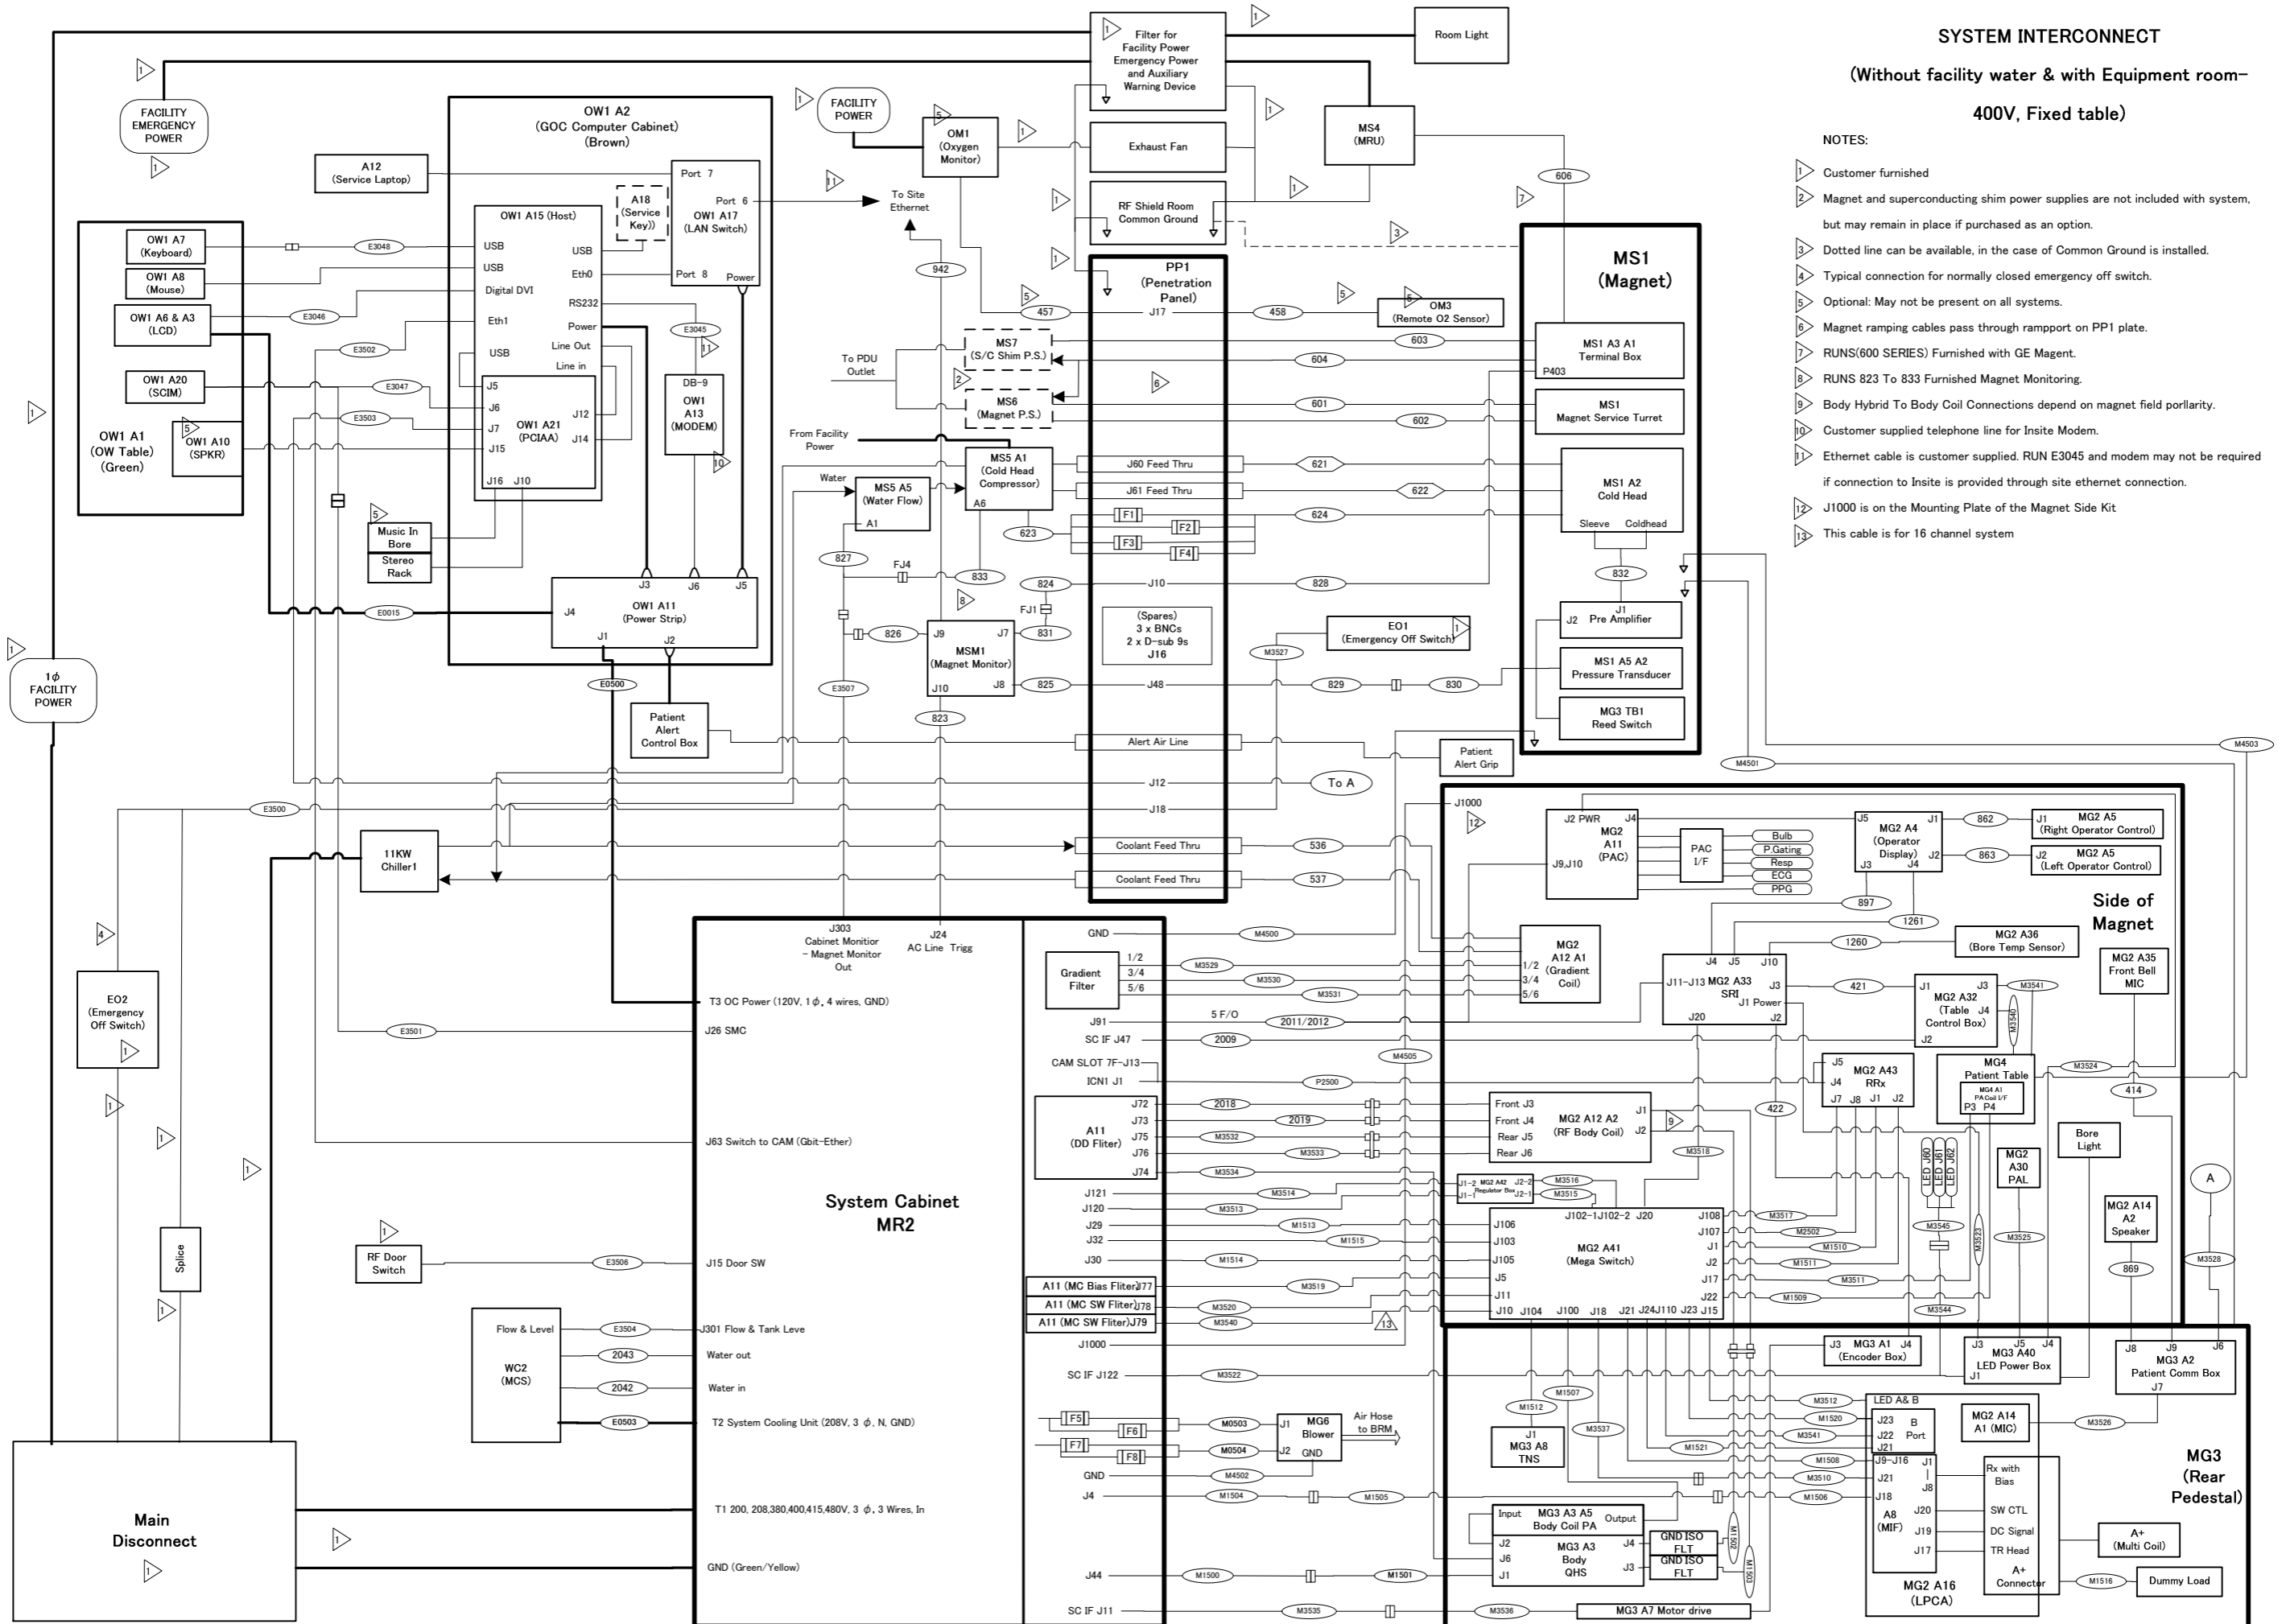

**SYSTEM INTERCONNECT**

(Without facility water & with Equipment room-  
400V, Fixed table)

**NOTES:**


- 1 Customer furnished
- 2 Magnet and superconducting shim power supplies are not included with system, but may remain in place if purchased as an option.
- 3 Dotted line can be available, in the case of Common Ground is installed.
- 4 Typical connection for normally closed emergency off switch.
- 5 Optional: May not be present on all systems.
- 6 Magnet ramping cables pass through rampout on PP1 plate.
- 7 RUNS(600 SERIES) Furnished with GE Magent.
- 8 RUNS 823 To 833 Furnished Magnet Monitoring.
- 9 Body Hybrid To Body Coil Connections depend on magnet field porlarity.
- 10 Customer supplied telephone line for Insite Modem.
- 11 Ethernet cable is customer supplied. RUN E3045 and modem may not be required if connection to Insite is provided through site ethernet connection.
- 12 J1000 is on the Mounting Plate of the Magnet Side Kit
- 13 This cable is for 16 channel system

# SYSTEM INTERCONNECT

(Without facility water & Non Equipment room-  
400V, Fixed table)

### NOTES:

- 1 Customer furnished
- 2 Magnet and superconducting shim power supplies are not included with system, but may remain in place if purchased as an option.
- 3 Dotted line can be available, in the case of Common Ground is installed.
- 4 Typical connection for normally closed emergency off switch.
- 5 Optional: May not be present on all systems.
- 6 Magnet ramping cables pass through rampport on PP1 plate.
- 7 RUNS(600 SERIES) Furnished with GE Magent.
- 8 RUNS 823 To 833 Furnished Magnet Monitoring.
- 9 Body Hybrid To Body Coil Connections depend on magnet field porlarity.
- 10 Customer supplied telephone line for Insite Modem.
- 11 Ethernet cable is customer supplied. RUN E3045 and modem may not be required if connection to Insite is provided through site ethernet connection.
- 12 J1000 is on the Mounting Plate of the Magnet Side Kit
- 13 This cable is for 16 channel system

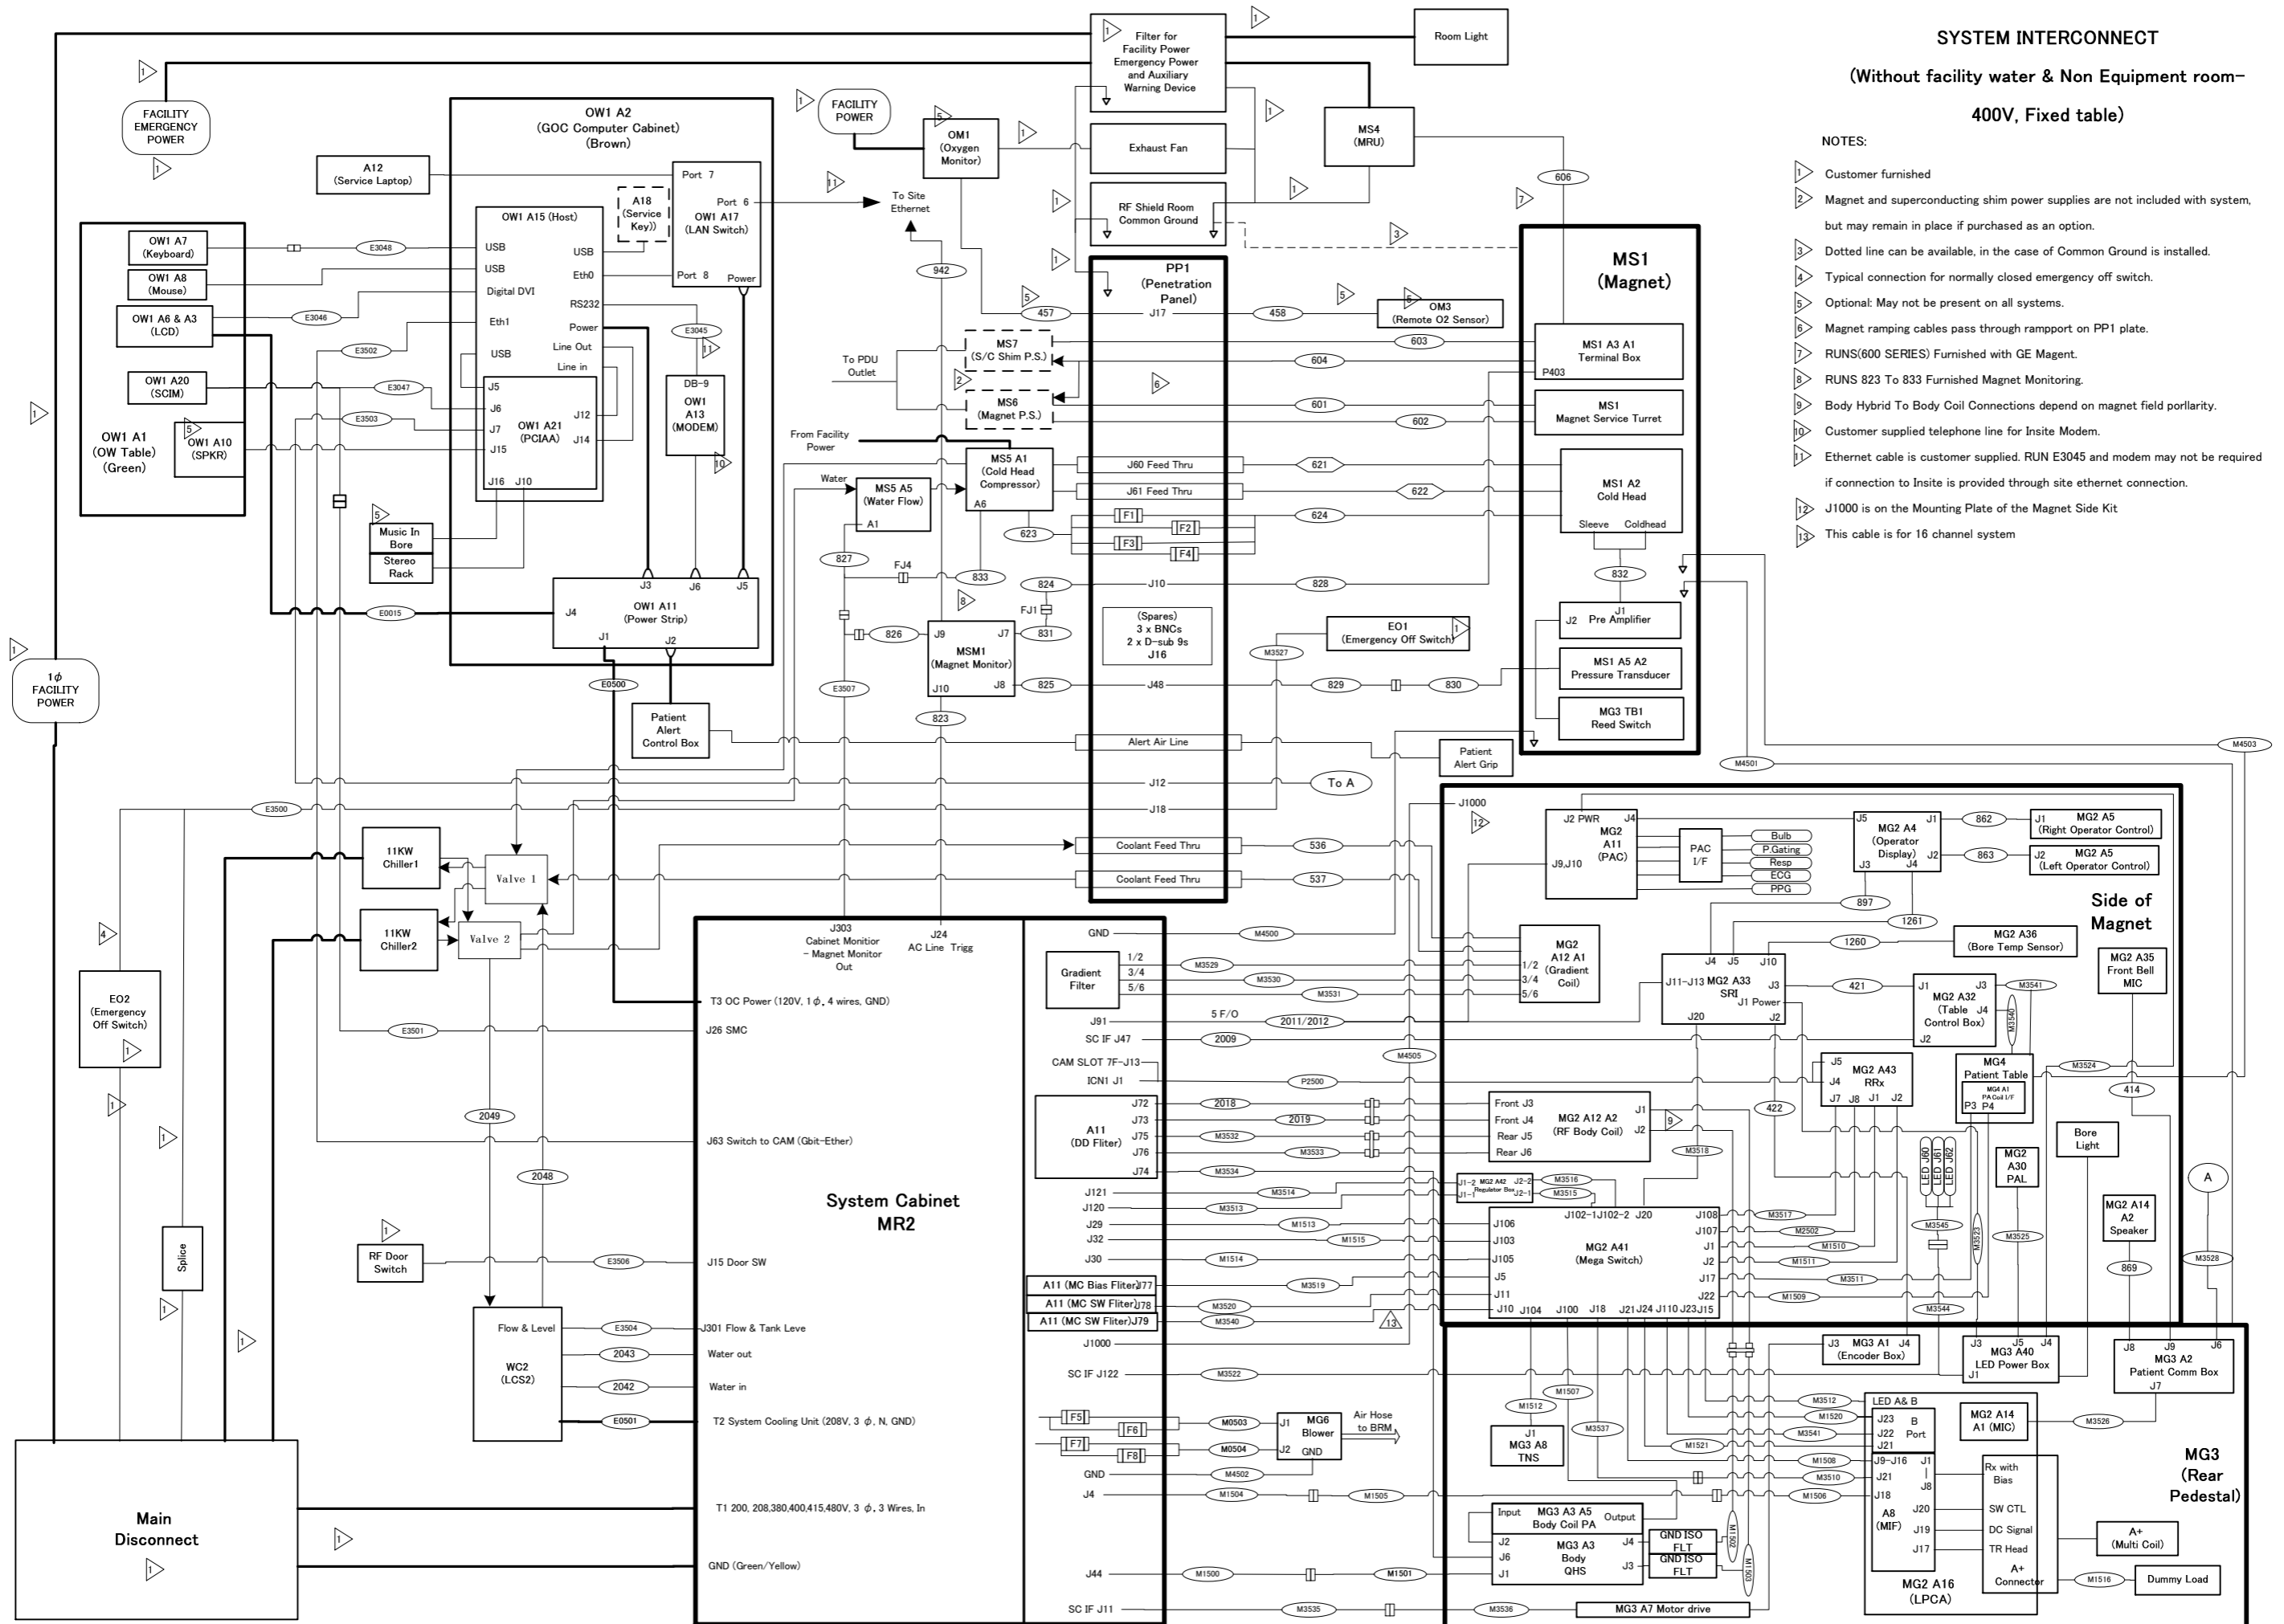

## System Cabinet MR2

## Side of Magnet

## MG3 (Rear Pedestal)



